

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
21 October 2004 (21.10.2004)

PCT

(10) International Publication Number  
**WO 2004/090565 A1**

(51) International Patent Classification<sup>7</sup>: **G01R 33/565**

**R., M.** [NL/NL]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(21) International Application Number:  
PCT/IB2004/050394

(74) Agent: **COHEN, Julius, S.**; Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(22) International Filing Date: 5 April 2004 (05.04.2004)

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
03100997.0 14 April 2003 (14.04.2003) EP

(71) Applicant (*for all designated States except US*): **KONINKLIJKE PHILIPS ELECTRONICS N.V.** [NL/NL]; Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).


(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR,

(72) Inventor; and

(75) Inventor/Applicant (*for US only*): **MENS, Wilhelmus,**

[Continued on next page]

(54) Title: **MAGNETIC RESONANCE IMAGING WITH HISTOGRAM-BASED PHASE CORRECTION**

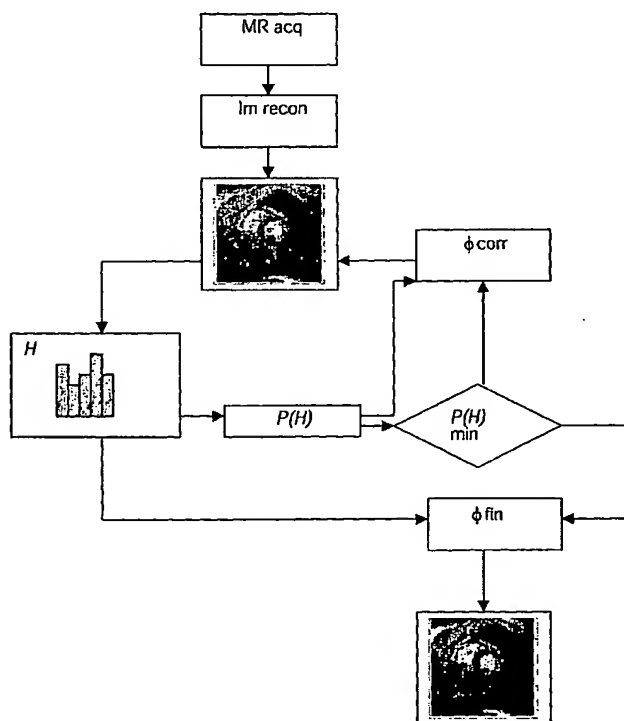

(57) Abstract: A magnetic resonance imaging system comprises reconstruction unit that is arranged to reconstruct a complex image of complex valued pixels from magnetic resonance signals. A compute a distribution of phase values of the complex image and to apply a phase correction to the complex image to form a corrected magnetic resonance image. The phase correction is controlled on the basis of the distribution of phase values of the complex image. Notably, the histogram power function is an effective indicator of the accuracy of the phase correction.

WO 2004/090565 A1



GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Declaration under Rule 4.17:**

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii)) for the following designations AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM,

ZW, ARIPO patent (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG)

**Published:**

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

2/pats

10/553327

JC20 Rec'd of PCTO 14 OCT 2005

1

## MAGNETIC RESONANCE IMAGING WITH HISTOGRAM-BASED PHASE CORRECTION

The invention pertains to a magnetic resonance imaging system which involves correction of phase values of the magnetic resonance image.

5                   Magnetic resonance imaging with phase correction is known from the paper '*A new phase correction method in NMR imaging based on autocorrelation and histogram analysis*' by C.B. Ahn and Z.H. Cho in IEEE Trans.MI 6(1987)32-36.

10                   The known magnetic resonance imaging proposes to correct the phase of the complex valued pixels by first making an estimate of the first order phase error. This first order phase error is the contribution to the phase error in a complex valued pixel that is linearly dependent on the position of the pixel in the complex image. This first order phase error is calculated from the autocorrelation between adjacent pixels. On the basis of the  
15                   estimate of the first order phase error a first-order phase error corrected image is derived. A histogram of phase values of the first-order phase error corrected image is formed. From the location of one peak in this histogram or of peaks being separated by 180° in this histogram, the zero-order phase error is estimated. This zero-order phase error is the overall contribution that is independent of the position of the pixel in the complex image.

20

                  An object of the invention is to provided an magnetic resonance imaging method in which phase errors having a complicated nature are corrected more accurately.

                  This object is achieved by a magnetic resonance imaging method according to  
25                   the invention comprising a reconstruction unit arranged to

- reconstruct a complex image of complex valued pixels from magnetic resonance signals
- compute a distribution of phase values of the complex image

- apply a phase correction to the complex image to form a corrected magnetic resonance image and
- control the phase correction on the basis of the distribution of phase values of the complex image.

5           According to the invention the phase correction is controlled on the basis of the distribution of the phase values of the complex image. It appears that the distribution of phase values is quite sensitive for the way the phase error depends on the position in the complex valued image. Consequently, the distribution of phase values is an accurate indicator for the kind of phase corrections to be effective and also for the accuracy of the result  
10 achieved by the phase correction actually applied. These and other aspects of the invention will be further elaborated with reference to the embodiments defined in the dependent Claims.

          Preferably, the distribution of phase values in the complex image is represented by a histogram of phase values. Generation of the histogram from the complex  
15 values of the pixels of the complex image requires very low computational effort and takes only a small memory capacity. Further, the features of the histogram appear to be very sensitive to the way the phase error varies over the complex valued image. Moreover, the features of the histogram also accurately indicate the accuracy achieved in correction of the phase error.

20           The use of test functions applied to the histogram enhances the sensitivity for particular patterns of variation of the phase error over the complex valued image. Further, the test function provides an easy indication of the accuracy of the correction in terms of a simple real valued number. Particularly suitable test functions are chosen from the class of functions  $f$  that satisfy:  $f(h) \geq h$  ( $h \geq 1$ ). These test functions enhance peaks in the histograms  
25 relative to broader structures. Accurate correction of the phase errors leads to peaks in the histogram and removes broad structures. As the test functions of this aspect of the invention favour peaks in the histogram, these test functions provide an accurate indication of the accuracy of the correction of the phase errors. Particularly good results are obtained when the histogram power function is employed as the test function. The histogram power function is  
30 defined as  $P(H) = \sum_{j \in H} h_j^2$ . Here  $H$  denotes the histogram and  $h_j$  is the number of phase-values in the  $j$ -th bin of the histogram  $H$ . The histogram power function strongly emphasises histograms having a few strong peaks and returns low values for histograms having mainly

broad features. Thus the histogram power function provides an effective test which indicates if the phase correction is accurate.

In a further implementation of the invention polynomial phase corrections are carried-out. Such polynomial phase corrections require low computational effort and require only a short computation time. Accordingly, several polynomial phase corrections can be tried within a short time and for the respective phase corrections the histogram is constructed and the histogram power function is computed. Then, the most effective correction is selected on the basis of the minimum histogram power function value. The respective polynomial phase corrections are easily effected just by adapting the polynomial coefficients of the polynomial phase corrections and re-iterating the phase correction with the adjusted polynomial coefficients. Preferably, the polynomial coefficients are adjusted so as to optimise the value of the test function of the histogram. These polynomial coefficients for which the test function of the histogram acquires its optimum value correspond to the most effective polynomial phase correction.

The computational efficiency of the phase correction is further improved in that the phase correction is adjusted by resetting the polynomial coefficients on the basis of a trial and improve algorithm so arrive at a set of polynomial coefficients that correspond to a phase distribution of which the test function of the histogram has it optimum value, notably the histogram power function, is minimum.

The corrected magnetic resonance image is practically void of artefacts caused by phase errors in the magnetic resonance signals. Accordingly, the corrected magnetic resonance image has a high diagnostic value in that the anatomy of the patient to be examined is imaged faithfully, even for small details with low contrast or low contrast-resolution.

The invention also relates to a magnetic resonance imaging method as defined in Claim 10. The magnetic resonance imaging method of the invention achieves accurate correction of phase errors in the complex valued image. The invention further relates to a computer programme as defined in Claim 11. The computer programme of the invention can be loaded into the reconstruction unit of the magnetic resonance imaging system.

Accordingly the reconstruction unit is able to perform accurate correction of phase errors in the complex valued image that is reconstructed from the magnetic resonance signals generated by the magnetic resonance imaging system.

These and other aspects of the invention will be elucidated with reference to the embodiments described hereinafter and with reference to the accompanying drawing wherein

5

Figure 1 shows a flow chart of an implementation of the method of the invention and

Figure 2 shows a schematic representation of a magnetic resonance imaging system in which the invention is employed.

10

Figure 1 shows a flow chart of an implementation of the method of the invention. The magnetic resonance imaging method of the invention involves acquisition (mr-acq) of magnetic resonance signals. From the acquired magnetic resonance signals, the complex image is reconstructed (Im-recon). For individual complex valued pixels of the complex image, the phase is computed. Then the phase-values for the pixels are binned into the histogram. That is, phase-values in pre-determined phase-intervals, the bins, are counted and the numbers of phase values in respective bins form the histogram  $H$ . From the histogram the histogram power function  $P(H) = \sum_{j \in H} h_j^2$  is computed and on the basis of the value of

the histogram power function a polynomial phase correction is selected and applied to the complex image. In an iterative way, again the histogram and its histogram power function are computed and a new polynomial phase correction is selected and applied to the current complex image. The iteration is ended when the histogram power function has its minimum value which indicates that the histogram contains a few strong peaks which indicates that the current phase correction is adequate. Optionally, a final phase correction can be performed on the basis of the histogram having the minimum histogram power function value. For example, the optional final phase correction may involve an accurate water-fat shift correction. This water-fat shift correction is based on the separation of two main peaks in the histogram.

30

Figure 2 shows a schematic representation of a magnetic resonance imaging system in which the invention is employed. The magnetic resonance imaging system includes a set of main coils 10 whereby the steady, uniform magnetic field is generated. The main coils are constructed, for example in such a manner that they enclose a tunnel-shaped

examination space. The patient to be examined is slid into this tunnel-shaped examination space. The magnetic resonance imaging system also includes a number of gradient coils 11, 12 whereby magnetic fields exhibiting spatial variations, notably in the form of temporary gradients in individual directions, are generated so as to be superposed on the uniform magnetic field. The gradient coils 11, 12 are connected to a controllable power supply unit 21. The gradient coils 11, 12 are energised by application of an electric current by means of the power supply unit 21. The strength, direction and duration of the gradients are controlled by control of the power supply unit. The magnetic resonance imaging system also includes transmission and receiving coils 13, 16 for generating the RF excitation pulses and for picking up the magnetic resonance signals, respectively. The transmission coil 13 is preferably constructed as a body coil 13 whereby (a part of) the object to be examined can be enclosed. The body coil is usually arranged in the magnetic resonance imaging system in such a manner that the patient 30 to be examined is enclosed by the body coil 13 when he or she is arranged in the magnetic resonance imaging system. The body coil 13 acts as a transmission antenna for the transmission of the RF excitation pulses and RF refocusing pulses. Preferably, the body coil 13 involves a spatially uniform intensity distribution of the transmitted RF pulses (RFS). The same coil or antenna is usually used alternately as the transmission coil and the receiving coil. Furthermore, the transmission and receiving coil is usually shaped as a coil, but other geometries where the transmission and receiving coil acts as a transmission and receiving antenna for RF electromagnetic signals are also feasible. The transmission and receiving coil 13 is connected to an electronic transmission and receiving circuit 15.

It is to be noted that it is alternatively possible to use separate receiving coils 16. For example, surface coils 16 can be used as receiving coils. Such surface coils have a high sensitivity in a comparatively small volume. The transmission coils, such as the surface coils, are connected to a demodulator 24 and the received magnetic resonance signals (MS) are demodulated by means of the demodulator 24. The demodulated magnetic resonance signals (DMS) are applied to a reconstruction unit. The receiving coil is connected to a preamplifier 23. The preamplifier 23 amplifies the RF resonance signal (MS) received by the receiving coil 16 and the amplified RF resonance signal is applied to a demodulator 24. The demodulator 24 demodulates the amplified RF resonance signal. The demodulated resonance signal contains the actual information concerning the local spin densities in the part of the object to be imaged. Furthermore, the transmission and receiving circuit 15 is connected to a modulator 22. The modulator 22 and the transmission and receiving circuit 15 activate the

transmission coil 13 so as to transmit the RF excitation and refocusing pulses. The reconstruction unit derives one or more image signals from the demodulated magnetic resonance signals (DMS), which image signals represent the image information of the imaged part of the object to be examined. The reconstruction unit 25 in practice is  
5 constructed preferably as a digital image processing unit 25 which is programmed so as to derive from the demodulated magnetic resonance signals the image signals which represent the image information of the part of the object to be imaged. The signal on the output of the reconstruction monitor 26, so that the monitor can display the magnetic resonance image. It is alternatively possible to store the signal from the reconstruction unit 25 in a buffer unit 27  
10 while awaiting further processing.

The reconstruction unit of the magnetic resonance imaging system according to the invention is also provided with a processing unit, for example in the form of a computer which includes a (micro)processor. The processing unit of the reconstruction unit is arranged to carry out the phase correction to the complex valued image on the basis of the  
15 distribution of phase values in the complex valued image, e.g. as represented by the histogram. To this end, the computer program according to the invention is loaded, for example, into the processing unit of the reconstruction unit 25.



## CLAIMS:

1. A magnetic resonance imaging system comprising a reconstruction unit arranged to
  - reconstruct a complex image of complex valued pixels from magnetic resonance signals
  - 5 - compute a distribution of phase values of the complex image
  - apply a phase correction to the complex image to form a corrected magnetic resonance image and
  - control the phase correction on the basis of the distribution of phase values of the complex image.
- 10 2. A magnetic resonance imaging system as claimed in Claim 1, wherein the distribution of phase values of the complex image is represented by a histogram of the phase values of the complex image.
- 15 3. A magnetic resonance imaging method as claimed in Claim 2, wherein the phase correction is controlled on the basis of a test function of the histogram.
4. A magnetic resonance imaging system as claimed in Claim 3 wherein the test function of the histogram discriminates, in particular enhances peaks, peaks in the histogram
- 20 from broader distributions.
5. A magnetic resonance imaging system as claimed in Claim 4, wherein the test function is formed by the histogram power function.
- 25 6. A magnetic resonance imaging system as claimed in Claim 1, wherein the reconstruction unit is arranged to make the phase correction on the basis of a polynomial phase correction, said polynomial being represented by its polynomial coefficients.

7. A magnetic resonance imaging method as claimed in Claim 6, wherein the reconstruction unit is arranged to control the phase correction by adjusting polynomial coefficients of the polynomial phase correction.
- 5 8. A magnetic resonance imaging system as claimed in Claim 3, wherein the reconstruction unit is arranged
- to make the phase correction on the basis of a polynomial phase correction and
  - control the phase correction by adjusting polynomial coefficients of the polynomial phase correction so as to optimise the test function.
- 10 9. A magnetic resonance imaging system as claimed in Claim 8, wherein the polynomial coefficients are adjusted by way of a trial and improve algorithm controlled on the basis of the test function.
- 15 10. A magnetic resonance imaging method wherein
- a complex image of complex valued pixels is reconstructed from magnetic resonance signals
  - a distribution of phase values of the complex image is computed
  - a phase correction is applied to the complex image to form a corrected magnetic
  - 20 resonance image and
  - the phase correction is controlled on the basis of the distribution of phase values of the complex image.
11. A computer programme comprising instructions to
- 25
- compute a distribution of phase values of a complex image
  - apply a phase correction to the complex image to form a corrected magnetic resonance image and
  - control the phase correction on the basis of the distribution of phase values of the complex image.

1/2

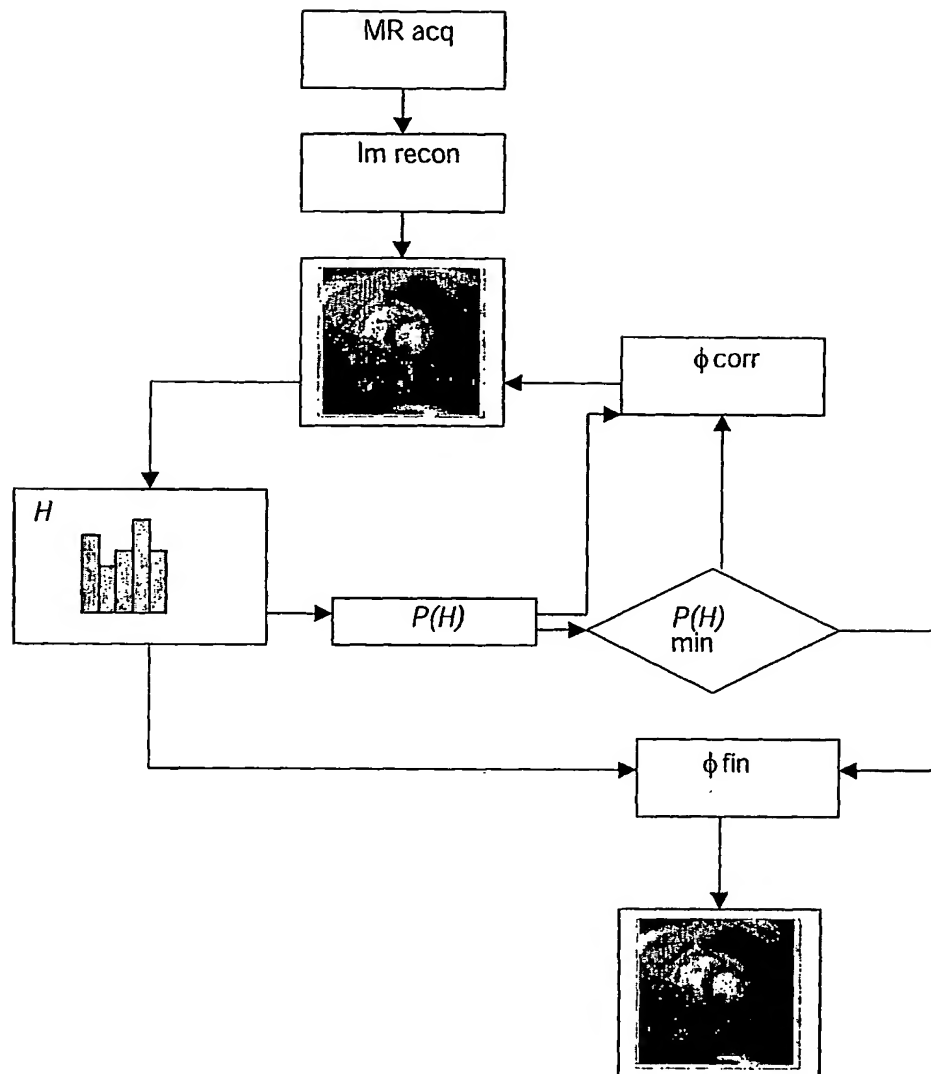


FIG.1

2/2

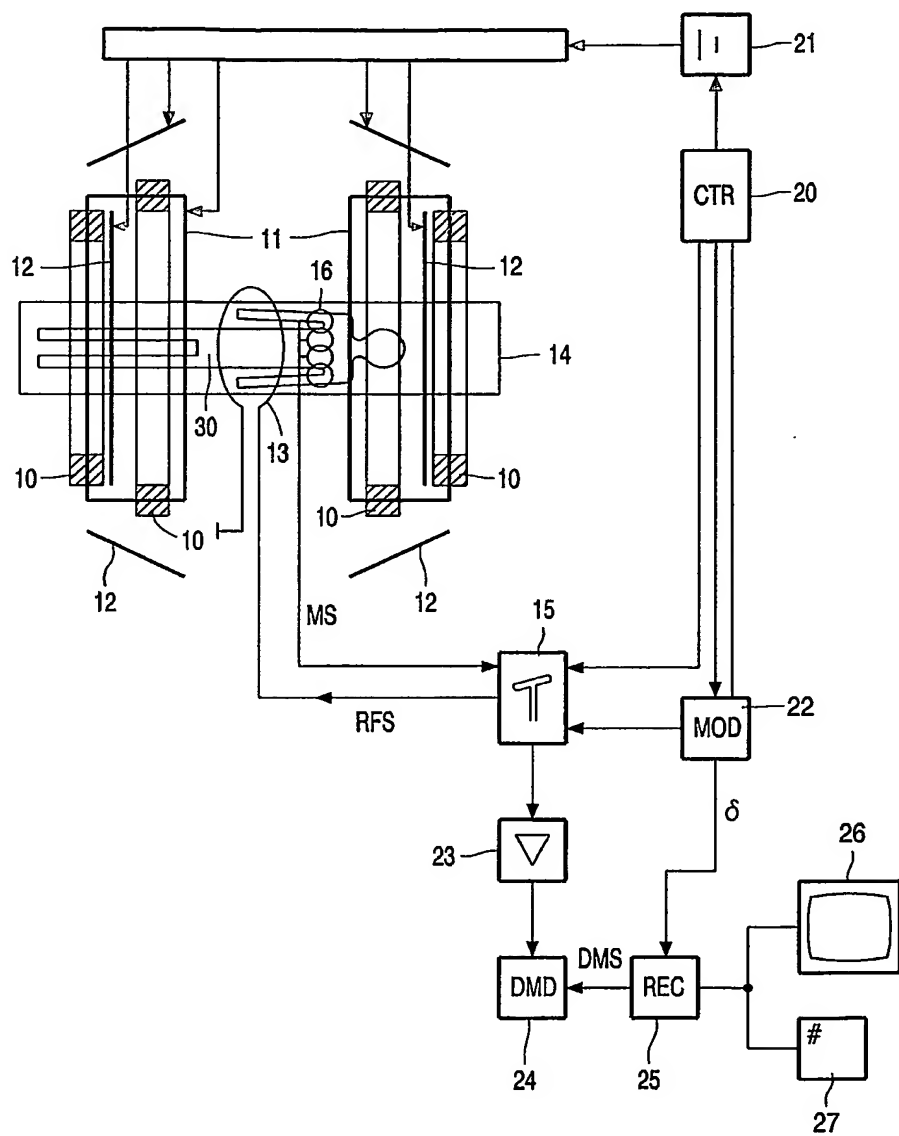


FIG. 2

# INTERNATIONAL SEARCH REPORT

onal Application No

IB2004/050394

A. CLASSIFICATION OF SUBJECT MATTER  
IPC 7 G01R33/565

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G01R

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, PAJ, WPI Data, BIOSIS, EMBASE, INSPEC

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>AHN C B ET AL: "NEW PHASE CORRECTION METHOD IN NMR IMAGING BASED ON AUTOCORRELATION AND HISTOGRAM ANALYSIS" IEEE TRANSACTIONS ON MEDICAL IMAGING, IEEE INC. NEW YORK, US, vol. MI-6, no. 1, March 1987 (1987-03), pages 32-36, XP000611030 ISSN: 0278-0062 cited in the application see chapters I and II</p> <p style="text-align: center;">-/--</p>	1-3,6,7, 10,11

☒ Further documents are listed in the continuation of box C.

☐ Patent family members are listed in annex.

\* Special categories of cited documents:

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

\*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

\*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

\*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

\*G\* document member of the same patent family

Date of the actual completion of the international search

16 July 2004

Date of mailing of the international search report

28/07/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel: (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Lersch, W

# INTERNATIONAL SEARCH REPORT

onal Application No

IB2004/050394

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>JUWHAN LIU ET AL: "AN AUTOMATIC PHASE CORRECTION METHOD IN NUCLEAR MAGNETIC RESONANCE IMAGING"</p> <p>JOURNAL OF MAGNETIC RESONANCE, ACADEMIC PRESS, ORLANDO, FL, US,</p> <p>vol. 86, no. 3,</p> <p>15 February 1990 (1990-02-15), pages 593-604, XP000132485</p> <p>ISSN: 1090-7807</p> <p>see the whole document</p>	<p>1-3,6,7, 10,11</p>
A	<p>FOXALL D L ET AL: "RAPID INTERACTIVE RECONSTRUCTION FOR ECHO PLANAR IMAGING"</p> <p>MAGNETIC RESONANCE IN MEDICINE, ACADEMIC PRESS, DULUTH, MN, US,</p> <p>vol. 42, no. 3, September 1999 (1999-09), pages 541-547, XP000859168</p> <p>ISSN: 0740-3194</p> <p>see pages 542-543</p>	<p>1,10,11</p>